

# 80PK-22

## *SureGrip™ Immersion Temperature Probe*

### *Instruction Sheet*

#### **⚠⚠ Warning**

**To avoid electrical shock, do not use this probe when voltages exceeding 24 V ac rms or 60 V dc are present. The probe tip is electronically connected to the output terminals.**

#### **Introduction**

The 80PK-22 SureGrip™ Immersion Temperature Probe is designed for use in liquids or gels. The probe can also be used as a general purpose temperature probe. The thermocouple junction is protected from tip to handle by an Inconel sheath. The 40-inch (1 meter) cable is terminated with a Type K miniature thermocouple connector with 0.792-mm (0.312-in) pin spacing. The 80PK-22 can be used with any temperature-measuring instrument that is designed to accept Type K thermocouples and has a miniature connector input.

#### *Note*

*The 80PK-22 is not recommended for use in food or beverage preparation. Use 80PK-25 for food preparation.*

#### **Specifications**

##### **Type**

K Standard grade Ni-Cr vs. Ni-Al (Chromel vs. Alumel)

##### **Measurement Range**

-40 °C to 1090 °C (-40 °F to 1994 °F)

##### **Accuracy**

(With respect to ANSI MC96.1-1982-Standard Limits of Error)

#### *Note*

*All error calculations should be done in °C, then scaled to °F.*

<b>Range</b>	<b>Accuracy (% of reading)</b>
-40 °C to 293 °C (-40 °F to 559.4 °F)	±2.2 °C
293 °C to 1090 °C (559.4 °F to 1994 °F)	±0.75 %

## ***Output***

@ 25 °C (77 °F) = 1.00 mV (reference junction @ 0 °C)

## ***Seebeck Coefficient***

@ 25 °C (77 °F) = 40.50  $\mu\text{V} / ^\circ\text{C}$

## ***Measurement Time***

(Time Constant): 3.0 seconds in 100 °C still water at sea level pressure. Complete step change equals 5 time constants (3.75 seconds).

## ***Maximum Voltage***

24 V ac rms or 60 V dc

## ***Maximum Temperature of Tip***

1090 °C (1994 °F)

## ***Sheath***

Material: Alloy 600

Dimensions:

Diameter: 3.175 mm (1/8 in)

Length: 212.725 mm (8.375 in)

## ***Grounding***

Junction welded to sheath.

## ***Cable***

Length: 40 inches (1 meter)

Insulation

Material: PVC

Maximum Temperature: 105 °C (220 °F)

Jacket Color: Gray

## ***Conductors***

Type: K

Size: AWG #24 stranded (7 strands of #32)

## ***Handle***

Material: Hytrel

Maximum Temperature: 125 °C (257 °F)

## ***Connector***

Type: Mini-thermocouple connector with .792 mm (0.312 in) pin spacing

Material: Yellow Hytrel

Maximum Temperature: 125 °C (257 °F)

## ***Overall Length***

31.75 cm (12.5 in) from probe tip to end of cable strain relief.

## ***Protection***

Class 3. Relates solely to insulation and grounding properties defined in IEC 348.

## **Measurement Considerations**

### **Instrument Compatibility**

The 80PK-22 is compatible with any temperature-measuring instrument that accepts Type K thermocouples, has a miniature thermocouple connector, and has cold reference junction compensation. Accuracy of the temperature-measuring instrument must be considered along with the 80PK-22 accuracy specification to determine the overall accuracy of the combination.

### **Temperature Limitations**

The probe tip of the 80PK-22 has a continuous temperature rating of 1090 °C (1994 °F). However the opposite end of the sheath nearest the handle should not be subjected to temperatures greater than 125 °C (257 °F). This is the maximum temperature limitation of the handle.

### **Media Limitations**

The sheath material of the 80PK-22 is Inconel, an alloy of chromium and nickel. It has excellent resistance to oxidation and corrosion at high temperatures, but it should not be used in the presence of sulfur above 537 °C (1000 °F).

### **Operation**

Use the 80PK-22 as follows:

1. Connect the 80PK-22 to a compatible Type K temperature measuring instrument using the miniature (0.312-inch pin spacing) thermocouple connector.
2. Turn on the measuring instrument, and select the appropriate range and scale.
3. Check the readout on the measuring instrument. With no heat or cold source applied to the tip of the probe, the measuring instrument should display the ambient (room) temperature. If the instrument does not read out properly, refer to "Troubleshooting".

### **Minimizing Thermal Shunting**

The 80PK-22 Immersion Probe should be inserted at least 6.35 cm (2.5 in) into the environment to be measured to minimize the shunting effect of the sheath.

### **Troubleshooting**

With no heat or cold applied to the probe, the measuring instrument should display the ambient temperature. If the measuring instrument does not read out properly, try the following:

1. Verify that the temperature-measuring instrument is designed to be used with Type K thermocouples. The temperature-measuring instrument should have a yellow input connector and / or be marked with a "K" either on the case or on the display.
2. Check for an open circuit indicator on the measuring instrument. Some temperature measuring instruments have a built-in circuit to indicate if the connected probe is open. (All Fluke Temperature-measuring instruments have this feature.) Refer to the owners manual accompanying the measuring instrument to see if this feature is available.

Short the two input pins of the measuring instrument with a piece of wire. If the instrument is functioning, it should indicate the ambient temperature.

- If you suspect a broken connection, use an ordinary ohmmeter to read the continuity of the probe from pin to pin. The ohmmeter should read 10 ohms or less if there is continuity.

## **Scale Conversions**

Use the following equation to convert °C to °F:

$$(^{\circ}\text{C} \times 1.8) + 32 = ^{\circ}\text{F}$$

Use the following equation to convert °F to °C:

$$(^{\circ}\text{F} - 32) \times 0.5556 = ^{\circ}\text{C}$$

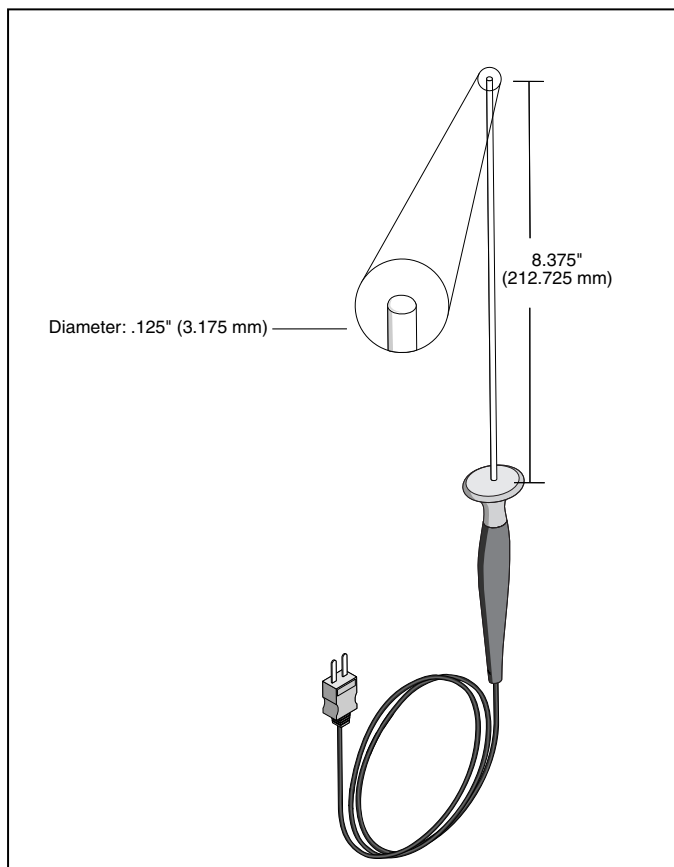


Figure 1. 80PK-22

bai01f.eps

## **Contacting Fluke**

For application or operation assistance, or information on Fluke products, call:

USA: 1-888-44-FLUKE (1-888-443-5853)

Canada: 1-800-36-FLUKE (1-800-363-5853)

Europe: +31 402-675-200

Japan: +81-3-3434-0181

Singapore: +65-738-5655

Anywhere in the world: +1-425-446-5500

For USA Service: 1-888-99-FLUKE

(1-888-993-5853)

Or, visit Fluke's Web site at [www.fluke.com](http://www.fluke.com).

To register your product, visit [register.fluke.com](http://register.fluke.com)

## ONE YEAR LIMITED WARRANTY

This Fluke product will be free from defects in material and workmanship for one year from the date of purchase. This warranty does not cover fuses, disposable batteries, or damage from accident, neglect, misuse, alteration, contamination, or abnormal conditions of operation or handling. Resellers are not authorized to extend any other warranty on Fluke's behalf. To obtain service during the warranty period, contact your nearest Fluke authorized service center to obtain return authorization information, then send the product to that Service Center with a description of the problem.

**THIS WARRANTY IS YOUR ONLY REMEDY. NO OTHER WARRANTIES, SUCH AS FITNESS FOR A PARTICULAR PURPOSE, ARE EXPRESSED OR IMPLIED. FLUKE IS NOT LIABLE FOR ANY SPECIAL, INDIRECT, INCIDENTAL OR CONSEQUENTIAL DAMAGES OR LOSSES, ARISING FROM ANY CAUSE OR THEORY.** Since some states or countries do not allow the exclusion or limitation of an implied warranty or of incidental or consequential damages, this limitation of liability may not apply to you.

Fluke Corporation  
P.O. Box 9090  
Everett, WA 98206-9090  
U.S.A.

Fluke Europe B.V.  
P.O. Box 1186  
5602 BD Eindhoven  
The Netherlands



Компания «ЭлектроПласт» предлагает заключение долгосрочных отношений при поставках импортных электронных компонентов на взаимовыгодных условиях!

Наши преимущества:

- Оперативные поставки широкого спектра электронных компонентов отечественного и импортного производства напрямую от производителей и с крупнейших мировых складов;
- Поставка более 17-ти миллионов наименований электронных компонентов;
- Поставка сложных, дефицитных, либо снятых с производства позиций;
- Оперативные сроки поставки под заказ (от 5 рабочих дней);
- Экспресс доставка в любую точку России;
- Техническая поддержка проекта, помощь в подборе аналогов, поставка прототипов;
- Система менеджмента качества сертифицирована по Международному стандарту ISO 9001;
- Лицензия ФСБ на осуществление работ с использованием сведений, составляющих государственную тайну;
- Поставка специализированных компонентов (Xilinx, Altera, Analog Devices, Intersil, Interpoint, Microsemi, Aeroflex, Peregrine, Syfer, Eurofarad, Texas Instrument, Miteq, Cobham, E2V, MA-COM, Hittite, Mini-Circuits, General Dynamics и др.);

Помимо этого, одним из направлений компании «ЭлектроПласт» является направление «Источники питания». Мы предлагаем Вам помощь Конструкторского отдела:

- Подбор оптимального решения, техническое обоснование при выборе компонента;
- Подбор аналогов;
- Консультации по применению компонента;
- Поставка образцов и прототипов;
- Техническая поддержка проекта;
- Защита от снятия компонента с производства.



#### Как с нами связаться

**Телефон:** 8 (812) 309 58 32 (многоканальный)

**Факс:** 8 (812) 320-02-42

**Электронная почта:** [org@eplast1.ru](mailto:org@eplast1.ru)

**Адрес:** 198099, г. Санкт-Петербург, ул. Калинина, дом 2, корпус 4, литера А.