

AC Outlet Analyzer and Wrist Strap Tester Installation, Operation and Maintenance



Made in the
United States of America



Figure 1. Desco 98132 AC Outlet Analyzer and Wrist Strap Tester



Figure 2. Desco 98131 AC Outlet Analyzer and Wrist Strap Tester

Description

The Desco AC Outlet Analyzer and Wrist Strap Tester verifies the proper wiring of AC outlets, provides a grounding point, and tests the path-to-ground integrity of an operator's wrist strap. Visual and audible indicators display pass and fail conditions for the outlet and pass condition for the wrist strap. When plugged into an AC outlet, the green LED illuminates to confirm that both the outlet's wiring is correct and the path to equipment ground via the equipment grounding conductor is intact. The banana jack provides a grounding point for wrist straps. An operator that is wearing and using the grounding point can touch the metal button to determine if the operator's wrist strap will act as a path-to-ground and ensure the presence of a current-limiting resistor in the wrist strap.

The factory test ranges are set to:

Wrist Straps: 750 kilohms and 35 megohms

Use the AC Outlet Analyzer and Wrist Strap Tester to fulfill the S6.1 Section 6.3.1 requirement. "The hot, neutral, and equipment grounding conductor shall be verified to be in the proper wiring orientation in accordance with the National Electric Code (ANSI/NFPA-70)." (Grounding ANSI/ESD S6.1 section 6.3.1 Equipment Grounding Conductor)

"Typical test programs recommend that wrist straps that are used daily should be tested daily." (ESD Handbook ESD TR20.20 section 5.3.2.4.4)

The AC Outlet Analyzer and Wrist Strap Tester is available in two models:

| Item | Input Voltage | Plug Type |
|-----------------------|---------------|-----------------------|
| 98132 | 100-120 VAC | North America / Japan |
| 98131 | 220 VAC | Asia / UK |

Packaging

- 1 AC Outlet Analyzer and Wrist Strap Tester
- 1 Certificate of Calibration

Features and Components

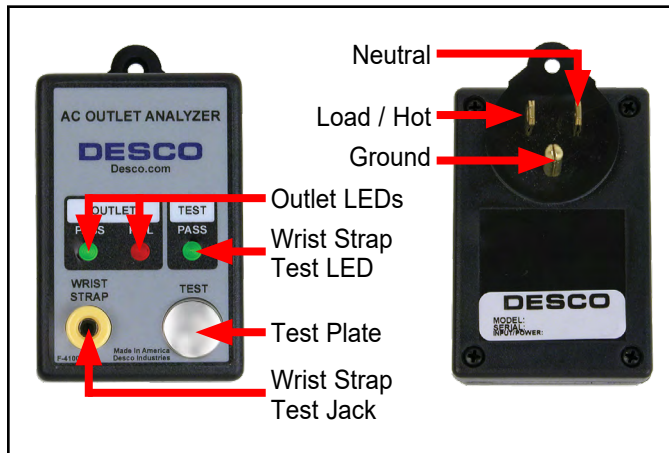


Figure 3. 98132 features and components

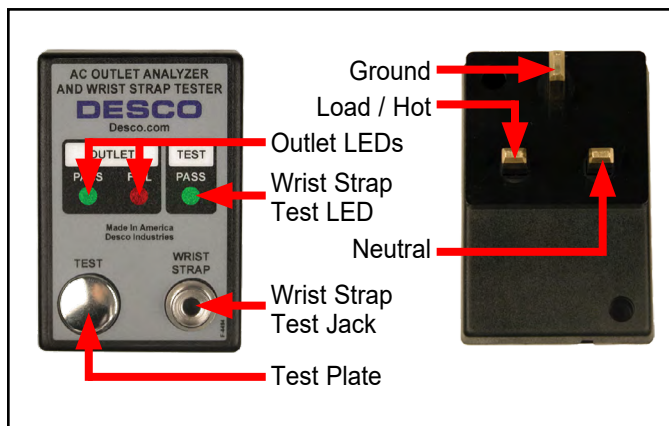


Figure 4. 98131 features and components

Installation

Performing an AC Outlet Test

Plug the AC Outlet Analyzer into a proper electrical outlet. The unit will indicate the condition of the electrical outlet via the Outlet LEDs.

- The green LED will illuminate if the outlet's wiring is correct and the path to equipment ground via the equipment grounding conductor is intact.
- The red LED will illuminate and the alarm will sound if the outlet's wiring is incorrect and/or the path to equipment ground via the equipment grounding conductor is not intact.

Operation

Performing a Wrist Strap Test

1. Use the wrist strap test jack to ground the operator's wrist strap.
2. While wearing the wrist strap, touch the tester's test plate to determine if the operator's wrist strap will act as a path-to-ground and ensure the presence of a current-limiting resistor in the wrist strap.

A "PASS" test result is indicated by illumination of the green TEST LED. A "FAIL" test result is indicated if the LED does not illuminate.

If your ESD test fails, check your wrist strap to ensure it is being worn correctly and/or needs to be replaced.

NOTE: Failures may be caused by dry skin or minimal sweat layer. For wrist straps, try using an approved dissipative hand lotion such as [Menda Reztore® ESD Hand Lotion](#) to your wrist prior to use.

The AC Outlet Analyzer and Wrist Strap Tester may also be used to test smocks or garments that feature a grounding mechanism for operators using a coil cord connection.

Calibration

Verifying the Wrist Strap Tester

A. LOW FAIL - Connect a 675 kilohm resistor @ 5% tolerance between the Wrist Strap Test Jack and the Test Plate. The Wrist Strap Test LED will momentarily illuminate then turn off. This test confirms the LOW FAIL point.

B. LOW PASS - Connect a 825 kilohm resistor @ 5% tolerance between the Wrist Strap Test Jack and the Test Plate. The Wrist Strap Test LED will remain illuminated until the resistor is removed from the Test Plate. This test confirms the LOW PASS point.

C. HIGH PASS - Connect a 32 megohm resistor @ 5% tolerance between the Wrist Strap Test Jack and the Test Plate. The Wrist Strap Test LED will remain illuminated until the resistor is removed from the Test Plate. This test confirms the HIGH PASS point.

D. HIGH FAIL - Connect a 40 megohm resistor @ 5% tolerance between the Wrist Strap Test Jack and the Test Plate. The Wrist Strap Test LED should not illuminate. This test confirms the HIGH FAIL point.

Verifying the AC Outlet Analyzer

NOTE: The following procedure should only be done by someone familiar with voltage hazards. This procedure will work for 220VAC as long as the neutral and ground are referenced. 220VAC produced with out of phase 110VAC-Ground-110VAC will produce a FAIL result.

Isolate the ground plug from the tester by inserting it into a 3 to 2 plug adapter.

A. PASS OUTLET - Connect a 5 kilohm resistor @ 5% tolerance between the supply ground and tester ground. The PASS LED should remain illuminated until the resistor is removed. This test confirms the PASS point for the neutral-to-ground resistance.

B. FAIL OUTLET - Connect a 12.5 kilohm resistor @ 5% tolerance between the supply ground and tester ground. The FAIL LED should remain illuminated until the resistor is removed. This test confirms the FAIL point for the neutral-to-ground resistance.

Specifications

| | |
|-----------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------|
| Input Voltage and Frequency | 98132: 90-138 VAC, 50/60 Hz 98131: 187-253 VAC, 50/60 Hz |
| Current Drain | < 10 mA |
| Operating Temperature | 50 to 95°F (10 to 35°C) |
| Environmental Requirements | Indoor use only at altitudes less than 6500 ft. (2 km) Maximum relative humidity of 80% up to 85°F (30°C) decreasing linearly to 50% @ 85°F (30°C) |
| Operator Test Limits | 750 kilohms to 35 megohms |
| Test Voltage | 27 VDC |
| Long Term Drift | < 1%/decade |
| Dimensions | 98132: 2.0" x 3.0" x 1.3" (51 mm x 76 mm x 33 mm) 98131: 2.0" x 3.0" x 2.0" (51 mm x 76 mm x 51 mm) |
| Weight | 0.2 lbs (91 g) |
| Country of Origin | United States of America |

Limited Warranty, Warranty Exclusions, Limit of Liability and RMA Request Instructions

See the Desco Warranty -

Desco.com/Limited-Warranty.aspx




Компания «ЭлектроПласт» предлагает заключение долгосрочных отношений при поставках импортных электронных компонентов на взаимовыгодных условиях!

Наши преимущества:

- Оперативные поставки широкого спектра электронных компонентов отечественного и импортного производства напрямую от производителей и с крупнейших мировых складов;
- Поставка более 17-ти миллионов наименований электронных компонентов;
- Поставка сложных, дефицитных, либо снятых с производства позиций;
- Оперативные сроки поставки под заказ (от 5 рабочих дней);
- Экспресс доставка в любую точку России;
- Техническая поддержка проекта, помощь в подборе аналогов, поставка прототипов;
- Система менеджмента качества сертифицирована по Международному стандарту ISO 9001;
- Лицензия ФСБ на осуществление работ с использованием сведений, составляющих государственную тайну;
- Поставка специализированных компонентов (Xilinx, Altera, Analog Devices, Intersil, Interpoint, Microsemi, Aeroflex, Peregrine, Syfer, Eurofarad, Texas Instrument, Miteq, Cobham, E2V, MA-COM, Hittite, Mini-Circuits, General Dynamics и др.);

Помимо этого, одним из направлений компании «ЭлектроПласт» является направление «Источники питания». Мы предлагаем Вам помощь Конструкторского отдела:

- Подбор оптимального решения, техническое обоснование при выборе компонента;
- Подбор аналогов;
- Консультации по применению компонента;
- Поставка образцов и прототипов;
- Техническая поддержка проекта;
- Защита от снятия компонента с производства.

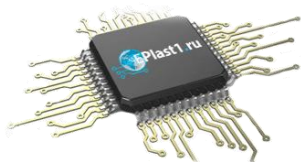

Как с нами связаться

Телефон: 8 (812) 309 58 32 (многоканальный)

Факс: 8 (812) 320-02-42

Электронная почта: org@eplast1.ru

Адрес: 198099, г. Санкт-Петербург, ул. Калинина, дом 2, корпус 4, литера А.